


Supplementary Figure S2

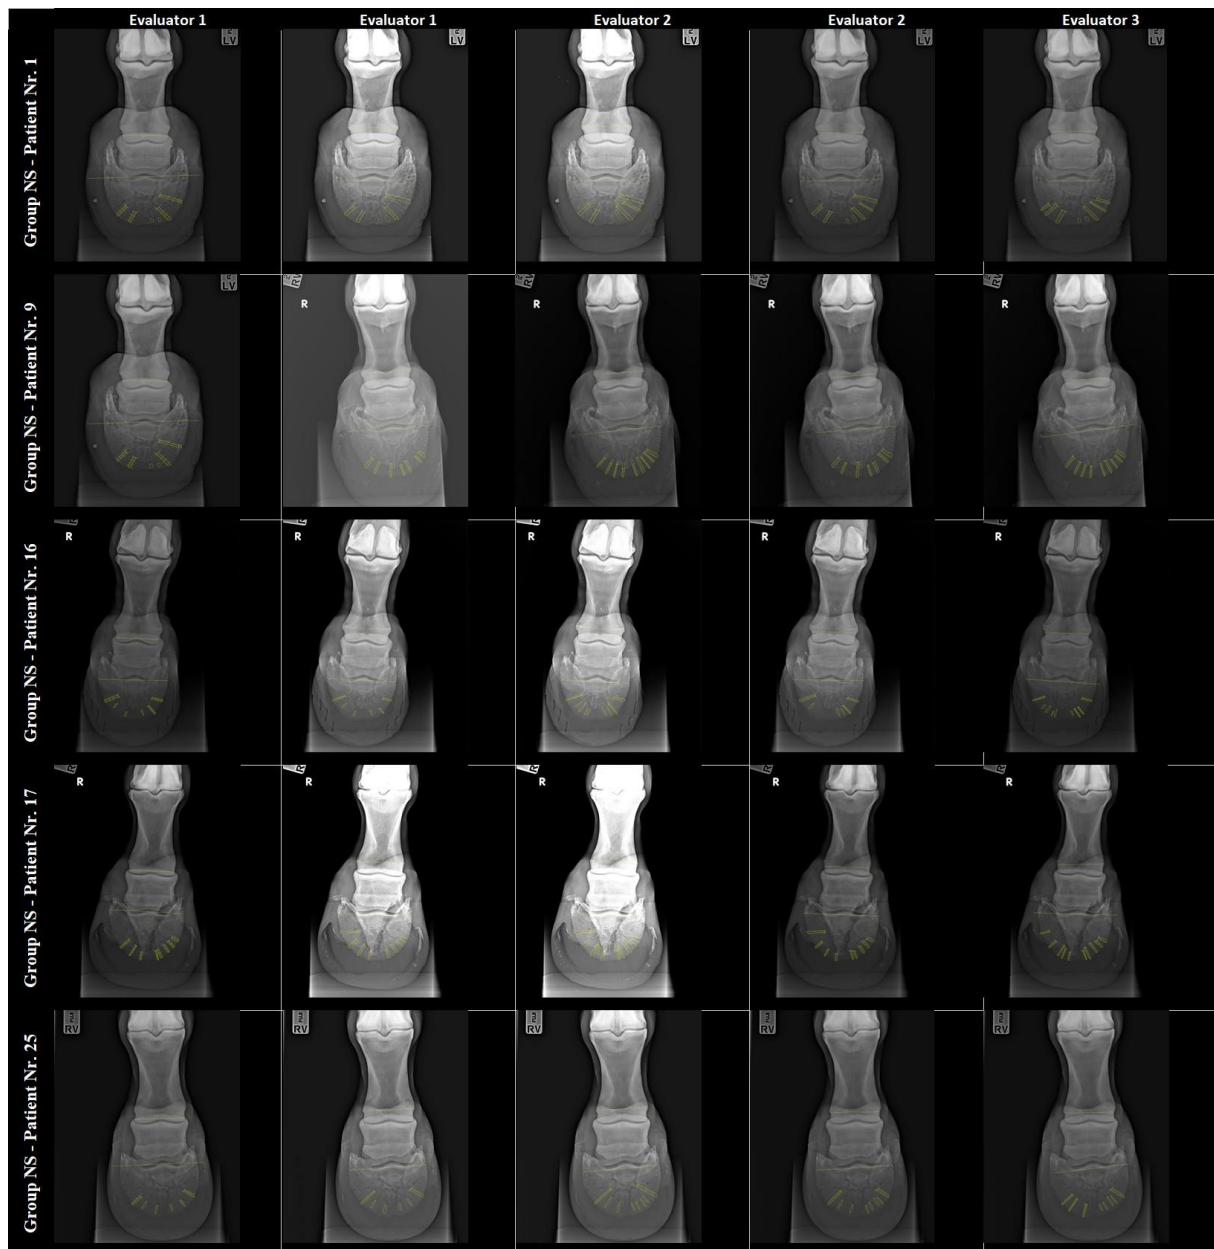

Supplementary Figure S2 – Oxspring (0° ; dorsoproximal–palmarodistal) radiographic views of 5 forefeet of 5 horses of Group NS (without laminitis) to illustrate the first measurements to test the repeatability and reliability of the software. Three human evaluators measured the same 5 radiographs, and evaluator 1 and 2 remeasured the same radiographs a second time.